


RING LOADING CONE



SUPPORT RING LOADING SYSTEM

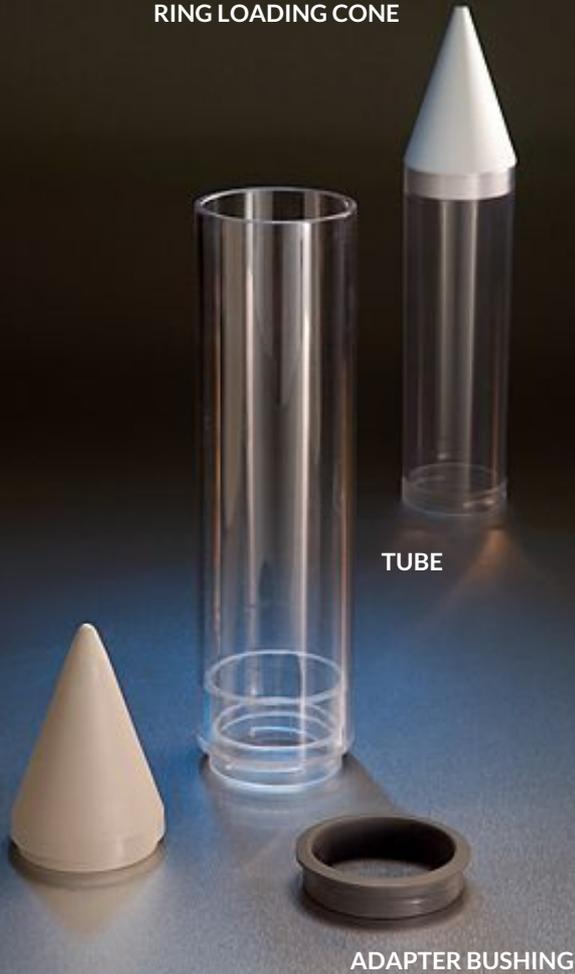

TENSION RINGS • RING LOADER USER INSTRUCTIONS

DO NOT WEAR A TENSION RING MORE THAN 30 MINUTES

The system will assist you in reaching a full and satisfying erection in most cases.

HOW TO LOAD THE TENSION RINGS

1. Start with the largest tension ring, and the adapter bushing. If you are unable to hold the erection with the larger ring, gradually use the next smallest tension ring until the ring is able to hold the erection.

2. Ensure the pump head and adapter bushing are removed from the penile tube. Place a towel on a firm, flat surface (waist high works best). Place the penile tube on the towel with the smooth end of the tube facing up. The towel will help the tube remain in place while loading the tension ring. (See Illustration #1.)

3. Place the loading cone into the smooth end of the penile tube. Generously lubricate the entire surface of the loading cone, top to bottom, and all around. Use only water soluble sealing gel. (See Illustration #2.)


4. Generously lubricate the entire surface of the cone with water soluble sealing gel, grasp the two handles of the tension ring as shown. Place your thumb tips on top of the tension ring next to the cone surface, press the tension ring down. Your thumb tips will glide along the surface of the cone. Place the tension ring near the end of the cylinder for easy off loading to the base of the penis. (Do not load the tension ring onto the cylinder by pulling the handles, they may tear.) (Illustration #3)

5. The tension ring will be transferred to the correct position on the penile tube at this time. If the ring fails to transfer to the tube, gently nudge the handles downward toward the tube and it will complete the transfer. (See Illustration #4.)

6. Remove the cone from the penile tube and attach the penile tube to the vacuum pump. Place the adapter bushing in the open end of the penile tube. If loose scrotal tissue travels into the tube use the smaller bushing (its fits inside the larger bushing). If you use more than one ring, choose a second ring and repeat steps 1 through 5.



ILLUS. #1

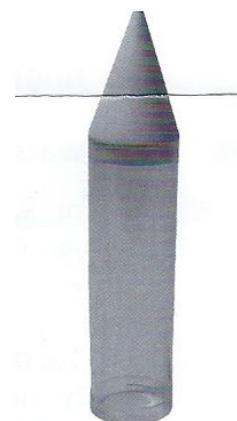

ILLUS. #2



ILLUS. #3



ILLUS. #4

USING A RING LOADER

Refer to the images to the right as you follow the instructions to use your Easy Loader.

1. Set the ring loading system on its flat end, with the fingers pointing upward. While turning the hex nut, slide it to the stop point toward the tip of the fingertips. This will bring the system fingers together. Lightly moisten the inside center of the tension ring with water soluble sealing gel.

Place the system fingertips inside the center of the tension ring. Slide the hex nut back to the handle of the system.

Turn the tension ring a quarter of a turn to help seat in place. Ensure the tension ring stays in place.

2. With the ring remaining on the loading system fingertips, grasp the system handle. Place the ring on the tip of the loading cone. Ensure the loading system is held straight up and down. Using your upper body along with your hand and wrist strength, quickly push down on the loading system, using one fluid motion until it comes to a stop.

To order additional rings, a ring loader, or other accessories to complement your vacuum therapy system:

Order online at: shopping.rejoynmedical.com

Or call 866-374-7640



Made in the U.S.A.
For single patient use only.

MANUFACTURED BY:

Pos-T-Vac, INC
2111 W. Wyatt Earp
Dodge City, KS 67801 USA
Ph. (620) 227-7434 Fax: (620)227-8474

EC/REP

CePartner4U
Esdoornlaan 13
3951 DB Maarn, 13 Netherlands
www.cepartner4u.eu



rejoyn
Medical Systems, Inc.